

DATA SHEET

SB02A


Safety barriers

SPECIAL FEATURES

- Three optimized safety barriers for intrinsically safe installation of SG-based sensors
- Intrinsic safety of the interconnection of the load cells confirmed by the conformity statement ExGuide 16 ATEX 0001 (Edition 3)
- Certification of barriers:
 - BAS 01 ATEX 7005,
 - IECEX BAS 09.0142,
 - IECEX BAS 17.0091X,
 - CML 21UKEX2898,
 - China SITIIAS CCC Ex Certificate,
 - India PESO (India) CCOE,
 - South Africa MASC,
 - Brasil TUV Rheinland Brazil
- ATEX/IECEX markings:
 - Ex II (1)G [Ex ia Ga] IIC
 - Ex II (1)D [Ex ia Da] IIIC
 - Ex I M1 [Ex ia Ma] I
 - Ex ec IIC T4 Gc
- Suitable for HBK amplifiers AD105D, PAD, WTX




DIMENSIONS

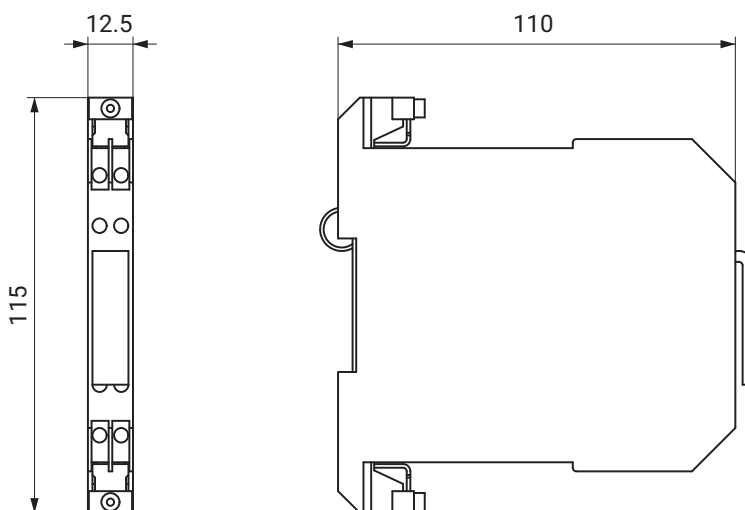

Dimensions in mm (1 mm = 0.03937 inches)

SPECIFICATIONS

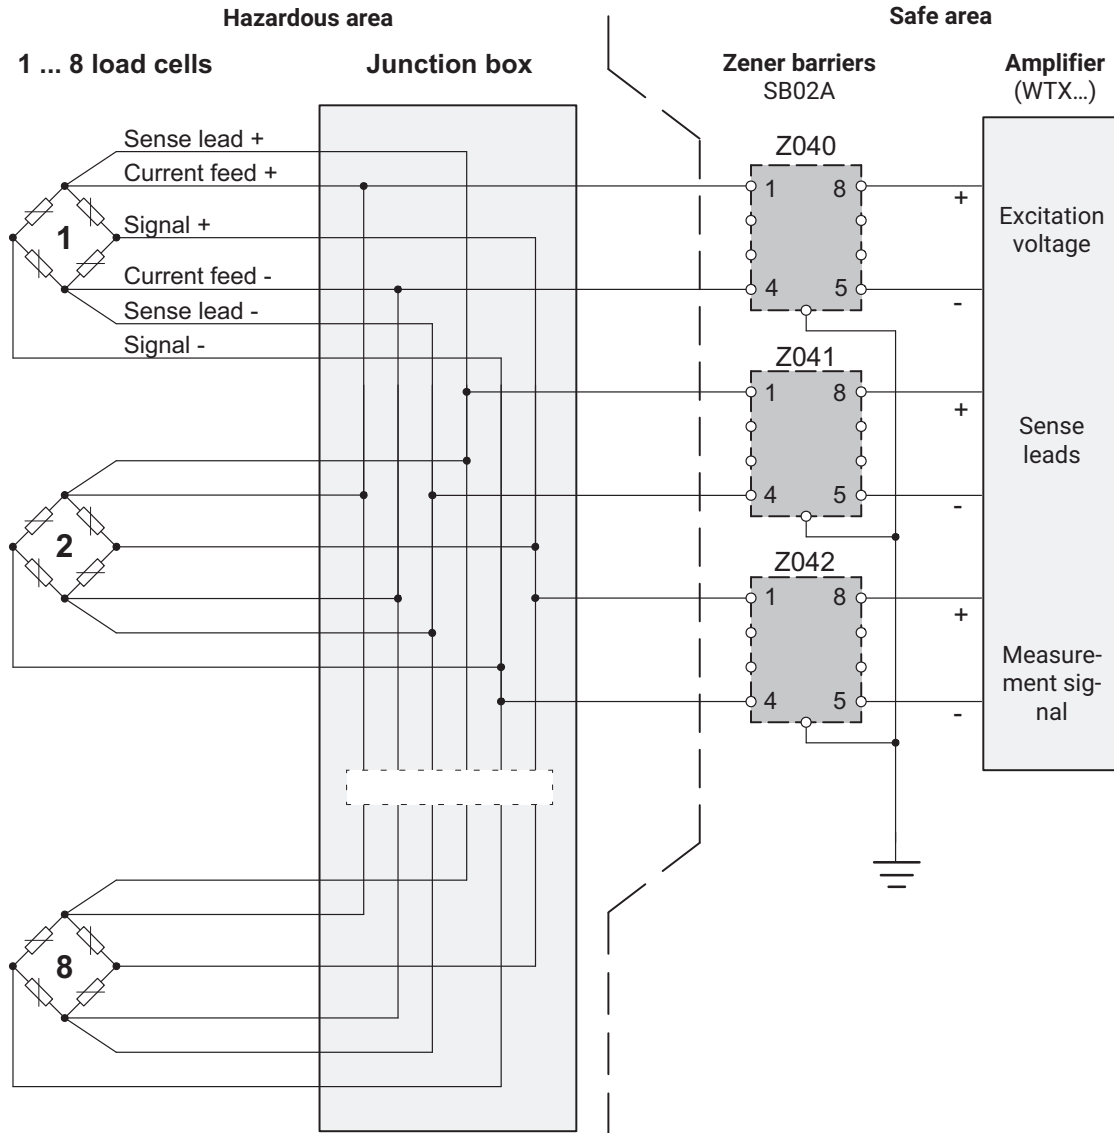

Notes:

Which device variants and which sensor excitation are precisely suitable can be found in the data sheets of the devices.

The maximum sensor cable lengths relate to the sensor cable and if available, the connection cable between the junction box of the sensors and the Zener barriers.

Approved cable types for the connection cable between junction box and Zener barriers:

- HBM:KAB7.5/00-2/2/2 (order no.: 1-CABE2/20, 1-CABE2/100) LF-ZYAECVY 3x2x0.14mm²
- LAPP: Li2YCYPMF 3x2x0.5mm²